

6099


PCB Piezotronics Inc. claims proprietary rights in the information disclosed hereon. Neither it nor any reproduction thereof will be disclosed to others without written consent of PCB Piezotronics Inc.

APPLICATION

NEXT ASS'Y	USED ON	VAR


REVISIONS

REV	DESCRIPTION	ECN	DATE	APP'D
A	REVISED PER ECR	19446	3/19/04	<i>Dm</i> 3/19/04

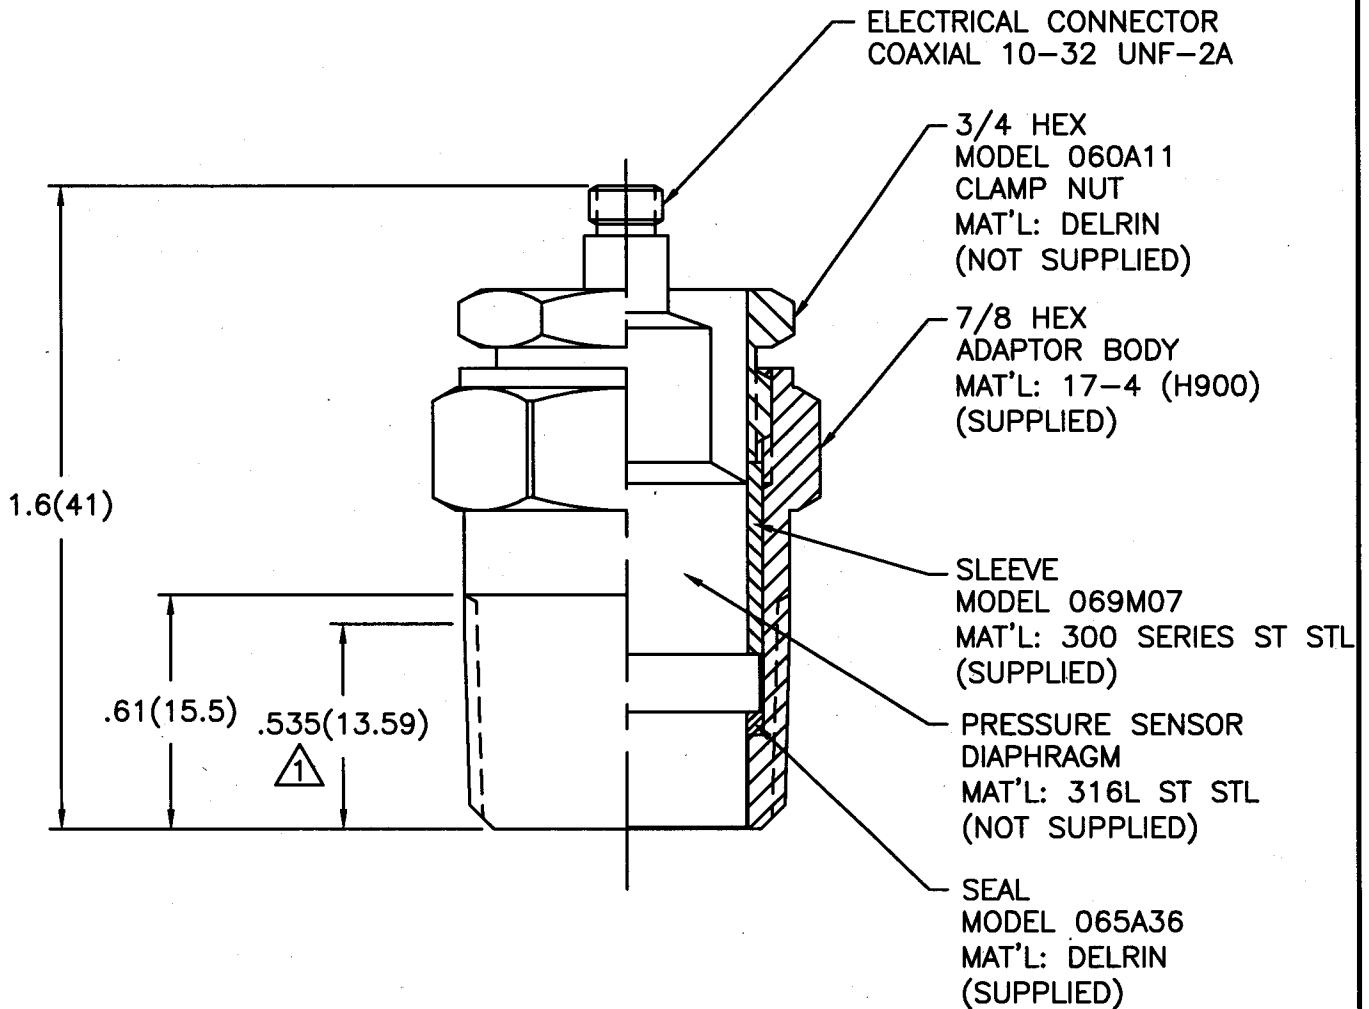

MOUNTING HOLE PREPERATION:

ϕ .718(ϕ 18.24)
 X .535(13.59) ∇ MIN.
 1/2-14 NPT
 X .535(13.59)

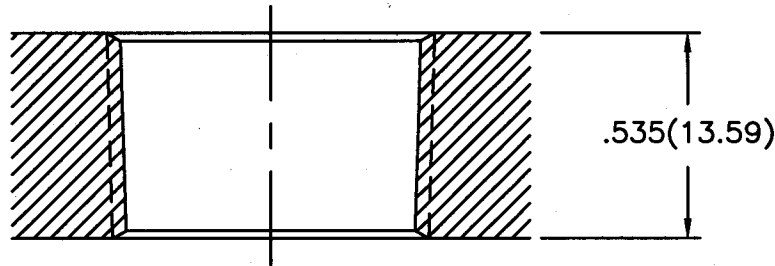

1. MAXIMUM INSERTION OF ADAPTOR INTO MOUNTING HOLE.
 2. USE PIPE JOINT COMPOUND TO ASSURE PRESSURE TIGHT SEAL.

UNLESS SPECIFIED TOLERANCES		DRAWN				MFG		PCB PIEZOTRONICS™	
DIMENSIONS IN INCHES	DIMENSIONS IN MILLIMETERS [IN BRACKETS]	FCB	3/24/04	MFG	PJL	3/24/04	3425 WALDEN AVE. DEPEW, NY 14043		
DECIMALS XX ±.01	DECIMALS X ±0.3	CHK'D	<i>Dm</i> 3/24/04	ENGR	<i>KCo</i> 3/24/04	(716) 684-0001 EMAIL: SALES@PCB.COM			
XXX ±.005	XX ±0.13	APP'D	<i>RF</i> 3/24/04	SALES	<i>DPC</i> 3/24/04	CODE IDENT. NO. 52681			
ANGLES ±2 DEGREES	ANGLES ±2 DEGREES	TITLE				DWG. NO.		6099	
FILLETS AND RADII .003 - .005	FILLETS AND RADII [0.07 - 0.13]	INSTALLATION DRAWING				SCALE: 2X		SHEET 1 OF 1	
DD011 REV. C 01/21/03		MODEL 062A07							
		PIPE THREAD ADAPTOR							